Adapting to Pentax Immersible GI Endoscopes**

With Screw In Air/Water & Suction Valves

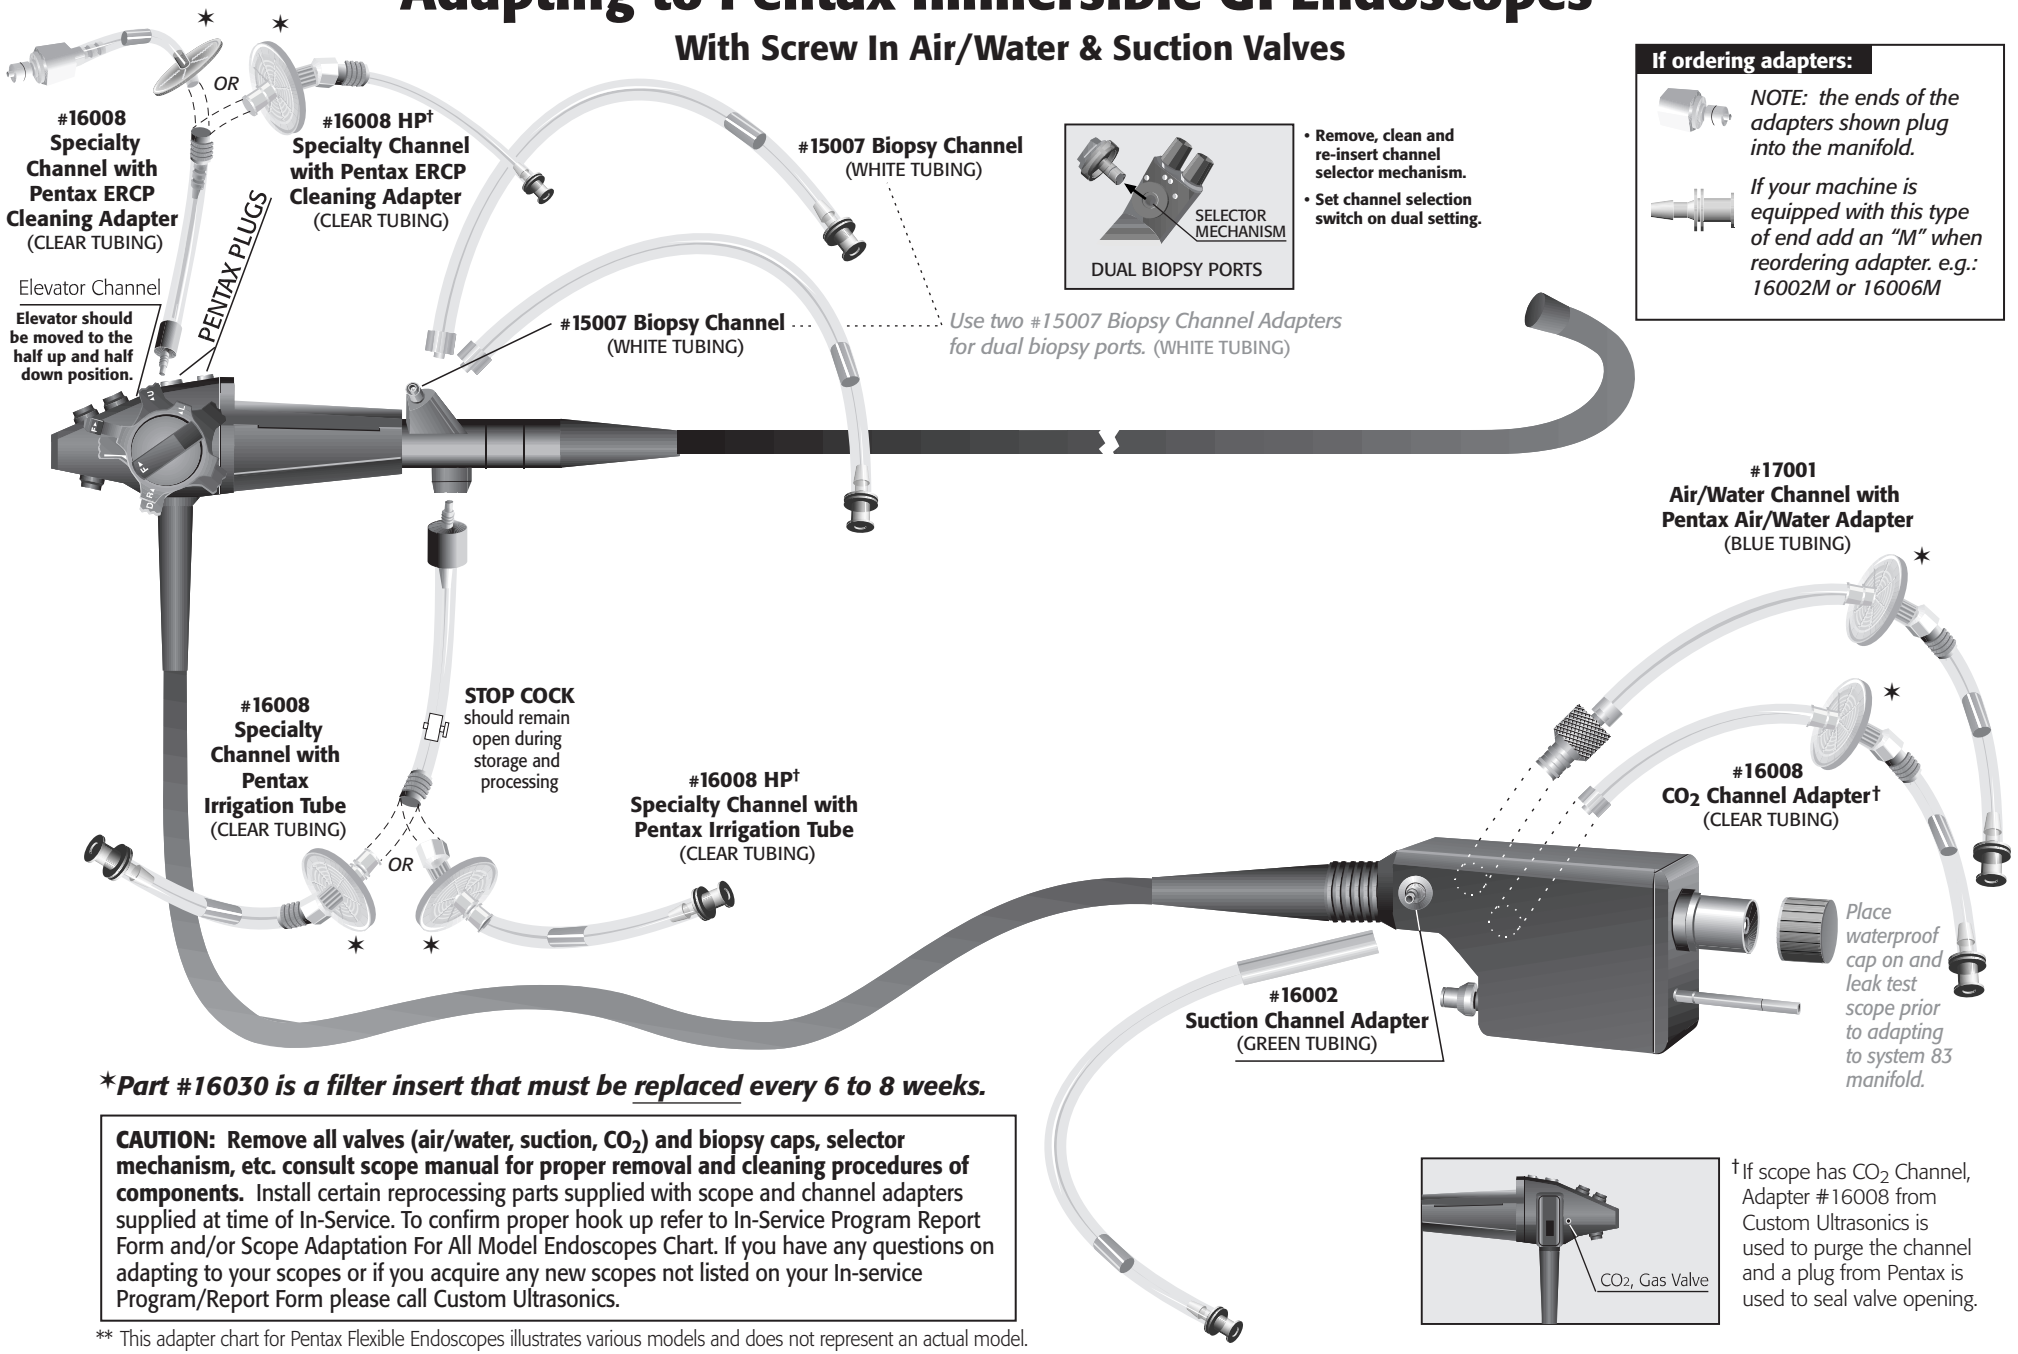
OR
#16008 Specialty Channel with Pentax ERCP Cleaning Adapter (CLEAR TUBING)
#16008 HP† Specialty Channel with Pentax ERCP Cleaning Adapter (CLEAR TUBING)
PENTAX PLUGS
Elevator Channel
Elevator should be moved to the half up and half down position.
#15007 Biopsy Channel (WHITE TUBING)
#15007 Biopsy Channel (WHITE TUBING)
Use two #15007 Biopsy Channel Adapters for dual biopsy ports. (WHITE TUBING)
SELECTOR MECHANISM
DUAL BIOPSY PORTS
• Remove, clean and re-insert channel selector mechanism.
• Set channel selection switch on dual setting.
If ordering adapters:
NOTE: the ends of the adapters shown plug into the manifold.
If your machine is equipped with this type of end add an "M" when reordering adapter. e.g.: 16002M or 16006M
#17001 Air/Water Channel with Pentax Air/Water Adapter (BLUE TUBING)
#16008 Specialty Channel with Pentax Irrigation Tube (CLEAR TUBING)
STOP COCK should remain open during storage and processing
#16008 HP† Specialty Channel with Pentax Irrigation Tube (CLEAR TUBING)
OR
#16008 CO2 Channel Adapter† (CLEAR TUBING)
Place waterproof cap on and leak test scope prior to adapting to system 83 manifold.
#16002 Suction Channel Adapter (GREEN TUBING)

✶***Part #16030 is a filter insert that must be replaced every 6 to 8 weeks.***

CAUTION: Remove all valves (air/water, suction, CO_2) and biopsy caps, selector mechanism, etc. consult scope manual for proper removal and cleaning procedures of components. Install certain reprocessing parts supplied with scope and channel adapters supplied at time of In-Service. To confirm proper hook up refer to In-Service Program Report Form and/or Scope Adaptation For All Model Endoscopes Chart. If you have any questions on adapting to your scopes or if you acquire any new scopes not listed on your In-service Program/Report Form please call Custom Ultrasonics.

† If scope has CO_2 Channel, Adapter #16008 from Custom Ultrasonics is used to purge the channel and a plug from Pentax is used to seal valve opening.

** This adapter chart for Pentax Flexible Endoscopes illustrates various models and does not represent an actual model.
† For machines that are equipped with High Pressure Ports use #16008 HP Specialty Channel.

Custom Ultrasonics INCORPORATED
P.O. Box 850 Buckingham, PA 18912 (215) 364-1477 FAX (215) 364-7674 www.customultrasonics.com

FEB2003-PEN(2)